

INCLUSIVE®

DENTAL IMPLANT SYSTEM



PRODUCT CATALOG

INTRODUCING THE INCLUSIVE® DENTAL IMPLANT SYSTEM

The Inclusive® Dental Implant System is the result of an expansive effort to offer clinicians and their patients a simple, convenient, affordable way to restore missing dentition. Choose between conventional-diameter or small-diameter implant assortments, supported by a wide array of restorative options, and discover a system that is streamlined for ease of use. From cementable or screw-retained single-tooth replacement to full-arch reconstruction with removable or fixed-removable prostheses, the Inclusive Dental Implant System can provide a predictable foundation for clinical success.

ABOUT THE MANUFACTURER

Prismatik Dentalcraft was established in 2006 with the mission of making implant dentistry the standard of care for edentulous patients across the economic spectrum. To realize this goal, we carefully assembled a team of experts with decades of combined experience in the design, engineering, and manufacture of dental implants. With a support staff of highly respected researchers, material scientists, clinical specialists, and dental technicians, Prismatik is dedicated to advancing implant therapies by combining proven treatment protocols with progressive materials, technologies, and techniques.

EXPERT PERSONNEL



Our team of experts have decades of combined experience in the design and manufacture of dental implants.

STATE-OF-THE-ART EQUIPMENT



Our Swiss-type lathes and multi-axis milling machines are ideal for implants and prosthetics requiring extreme precision.

MADE IN THE USA



Our ISO-certified facility in Irvine, Calif. operates under FDA Current Good Manufacturing Practices (CGMPs).

CONTENTS

4	INCLUSIVE TAPERED IMPLANT TECHNICAL SPECIFICATIONS
5	TAPERED IMPLANTS
6	HEALING COMPONENTS
7	IMPRESSION COMPONENTS
8	STOCK ABUTMENTS
9	SCREWS & GUIDE PINS
10	MULTI-UNIT ABUTMENT SYSTEM
12	LOCATOR® ABUTMENT SYSTEM
14	SURGICAL KIT OVERVIEW
15	PROSTHETIC KIT OVERVIEW
16	DRILLS & TAPS
17	INSTRUMENTATION
18	INCLUSIVE MINI IMPLANT TECHNICAL SPECIFICATIONS
19	MINI IMPLANTS
20	PROSTHETIC COMPONENTS
21	SURGICAL KIT OVERVIEW
23	INSTRUMENTATION
24	IMPLANT PACKAGING
25	POLICIES AND WARRANTY
26	PARTS INDEX

*Inclusive® is a registered trademark of Prismatic Dentalcraft, Inc.
LOCATOR is a registered trademark of Zest Anchors, LLC.*

Copyright © 2022, Prismatic Dentalcraft, Inc. Prismatic Dentalcraft, Inc. is not responsible for any damages or other liabilities (including attorney fees) resulting, or claimed to result in whole or in part, from actual or alleged problems arising out of the use of this information. The techniques, procedures and theories presented herein are provided in good faith and believed to be correct as of the date hereof. Any dental professional viewing this presentation must make his or her own decisions about the use of the materials and techniques for specific situations.

No representations as to the completeness or accuracy of this information is given, and no representations or warranties, either expressed or implied, of merchantability, fitness for a particular purpose or of any other nature are made here under with respect to the information or the product to which information refers.

INCLUSIVE®

TAPERED IMPLANT SYSTEM



3.2 mmD
3.0 mmP
conical connection



3.7 mmD
3.5 mmP




4.2 mmD
3.5 mmP



4.7 mmD
4.5 mmP





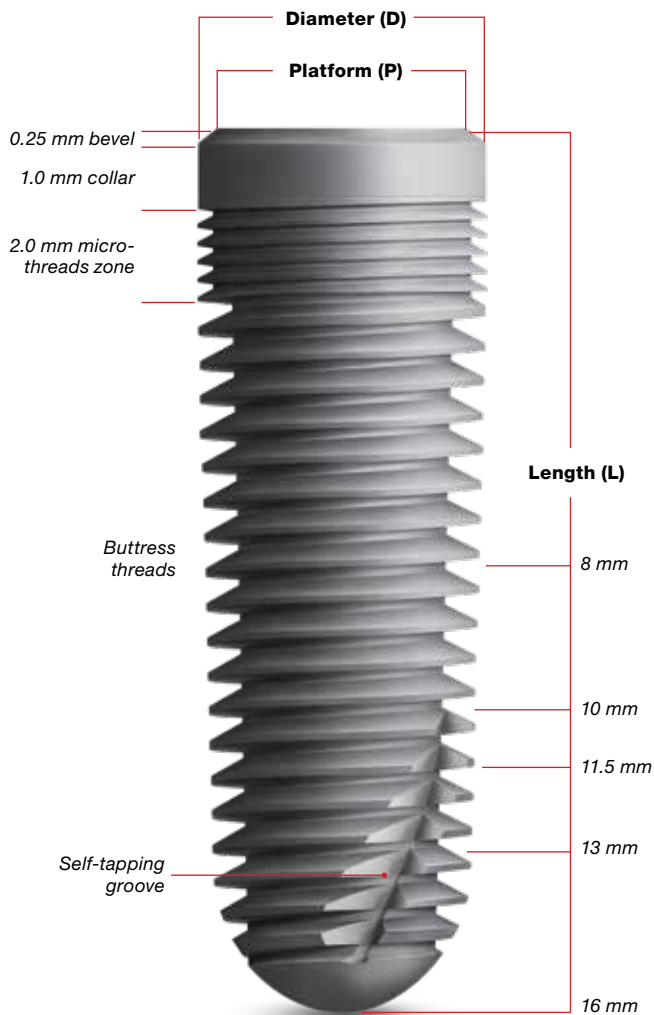






















5.2 mmD
4.5 mmP



TAPERED IMPLANTS



















Inclusive® Tapered Implants are machined from high-strength titanium alloy and incorporate design features for achieving high primary stability, crestal bone preservation, soft tissue maintenance, maximum bone-to-implant contact, natural root shape, and compatibility with popular prosthetic components and instrumentation. Inclusive Tapered Implants are available in five major diameters, each of which is available in up to five lengths. Three standard prosthetic platform sizes (3.0 mm, 3.5 mm, 4.5 mm) minimizes the number of system components and simplifies the restorative process.

	DESCRIPTION	CODE
INCLUSIVE® TAPERED IMPLANT		
 70-1070-IMP0035	 70-1070-IMP0036	 70-1070-IMP0032
 70-1070-IMP0033	 70-1070-IMP0034	
3.2 mmD x 8 mmL x 3.0 mmP 70-1070-IMP0035 3.2 mmD x 10 mmL x 3.0 mmP 70-1070-IMP0036 3.2 mmD x 11.5 mmL x 3.0 mmP 70-1070-IMP0032 3.2 mmD x 13 mmL x 3.0 mmP 70-1070-IMP0033 3.2 mmD x 16 mmL x 3.0 mmP 70-1070-IMP0034		
 70-1070-IMP0005	 70-1070-IMP0006	 70-1070-IMP0007
 70-1070-IMP0008	 70-1070-IMP0009	
3.7 mmD x 8 mmL x 3.5 mmP 70-1070-IMP0005 3.7 mmD x 10 mmL x 3.5 mmP 70-1070-IMP0006 3.7 mmD x 11.5 mmL x 3.5 mmP 70-1070-IMP0007 3.7 mmD x 13 mmL x 3.5 mmP 70-1070-IMP0008 3.7 mmD x 16 mmL x 3.5 mmP 70-1070-IMP0009		
 70-1070-IMP0026	 70-1070-IMP0027	 70-1070-IMP0028
 70-1070-IMP0029	 70-1070-IMP0030	
4.2 mmD x 8 mmL x 3.5 mmP 70-1070-IMP0026 4.2 mmD x 10 mmL x 3.5 mmP 70-1070-IMP0027 4.2 mmD x 11.5 mmL x 3.5 mmP 70-1070-IMP0028 4.2 mmD x 13 mmL x 3.5 mmP 70-1070-IMP0029 4.2 mmD x 16 mmL x 3.5 mmP 70-1070-IMP0030		
 70-1070-IMP0010	 70-1070-IMP0011	 70-1070-IMP0012
 70-1070-IMP0013	 70-1070-IMP0014	
4.7 mmD x 8 mmL x 4.5 mmP 70-1070-IMP0010 4.7 mmD x 10 mmL x 4.5 mmP 70-1070-IMP0011 4.7 mmD x 11.5 mmL x 4.5 mmP 70-1070-IMP0012 4.7 mmD x 13 mmL x 4.5 mmP 70-1070-IMP0013 4.7 mmD x 16 mmL x 4.5 mmP 70-1070-IMP0014		
 70-1070-IMP0015	 70-1070-IMP0016	 70-1070-IMP0017
 70-1070-IMP0018	 70-1070-IMP0019	
5.2 mmD x 8 mmL x 4.5 mmP 70-1070-IMP0015 5.2 mmD x 10 mmL x 4.5 mmP 70-1070-IMP0016 5.2 mmD x 11.5 mmL x 4.5 mmP 70-1070-IMP0017 5.2 mmD x 13 mmL x 4.5 mmP 70-1070-IMP0018 5.2 mmD x 16 mmL x 4.5 mmP 70-1070-IMP0019		

HEALING COMPONENTS







DESCRIPTION IMPLANT CODE

INCLUSIVE® TAPERED IMPLANT HEALING ABUTMENT

			3.0 mmP x 3.2 mmD x 3 mmH..... Ø3.2 70-1069-IMP0009
			3.0 mmP x 3.2 mmD x 5 mmH..... Ø3.2 70-1069-IMP0010
			3.0 mmP x 3.2 mmD x 7 mmH..... Ø3.2 70-1069-IMP0011
			3.0 mmP x 3.7 mmD x 3 mmH..... Ø3.2 70-1069-IMP0012
			3.0 mmP x 3.7 mmD x 5 mmH..... Ø3.2 70-1069-IMP0013
			3.0 mmP x 3.7 mmD x 7 mmH..... Ø3.2 70-1069-IMP0014
			3.5 mmP x 3.5 mmD x 3 mmH..... Ø3.7/4.2 70-1069-IMP0001
			3.5 mmP x 3.5 mmD x 5 mmH..... Ø3.7/4.2 70-1069-IMP0002
			3.5 mmP x 3.5 mmD x 7 mmH..... Ø3.7/4.2 70-1069-IMP0015
			3.5 mmP x 4.7 mmD x 3 mmH..... Ø3.7/4.2 70-1069-IMP0003
			3.5 mmP x 4.7 mmD x 5 mmH..... Ø3.7/4.2 70-1069-IMP0004
			3.5 mmP x 4.7 mmD x 7 mmH..... Ø3.7/4.2 70-1069-IMP0016
			4.5 mmP x 4.5 mmD x 3 mmH..... Ø4.7/5.2 70-1069-IMP0005
			4.5 mmP x 4.5 mmD x 5 mmH..... Ø4.7/5.2 70-1069-IMP0006
			4.5 mmP x 4.5 mmD x 7 mmH..... Ø4.7/5.2 70-1069-IMP0017
			4.5 mmP x 5.7 mmD x 3 mmH..... Ø4.7/5.2 70-1069-IMP0007
			4.5 mmP x 5.7 mmD x 5 mmH..... Ø4.7/5.2 70-1069-IMP0008
			4.5 mmP x 5.7 mmD x 7 mmH..... Ø4.7/5.2 70-1069-IMP0018

(Healing Abutments require a .050" hex instrument for placement - see page 17.)

INCLUSIVE® TAPERED IMPLANT TEMPORARY ABUTMENT

		3.0 mmP Ø3.2 70-1073-PRA0048
		Non-Engaging, 3.0 mmP Ø3.2 70-1073-PRA0047
		3.5 mmP Ø3.7/4.2 70-1073-PRA0022
		Non-Engaging, 3.5 mmP Ø3.7/4.2 70-1073-PRA0023
		4.5 mmP Ø4.7/5.2 70-1073-PRA0024
		Non-Engaging, 4.5 mmP Ø4.7/5.2 70-1073-PRA0025

(Temporary Abutments include Titanium Screw and Guide Pin.)

IMPRESSION COMPONENTS


DESCRIPTION IMPLANT CODE

INCLUSIVE® TAPERED IMPLANT TRANSFER COPING




70-1072-PRC0051

Closed-Tray, 3.0 mmP x 3.2 mmD Ø3.2 70-1072-PRC0051



70-1072-PRC0053

Closed-Tray, 3.0 mmP x 3.7 mmD Ø3.2 70-1072-PRC0053



70-1072-PRC0007

Closed-Tray, 3.5 mmP x 3.5 mmD Ø3.7/4.2 70-1072-PRC0007



70-1072-PRC0009

Closed-Tray, 3.5 mmP x 4.7 mmD Ø3.7/4.2 70-1072-PRC0009



70-1072-PRC0011


Closed-Tray, 4.5 mmP x 4.5 mmD Ø4.7/5.2 70-1072-PRC0011



70-1072-PRC0013

Closed-Tray, 4.5 mmP x 5.7 mmD Ø4.7/5.2 70-1072-PRC0013

(Closed-Tray Transfer Copings include Closed-Tray Screw.)



70-1072-PRC0052

Open-Tray, 3.0 mmP x 3.2 mmD Ø3.2 70-1072-PRC0052



70-1072-PRC0054

Open-Tray, 3.0 mmP x 3.7 mmD Ø3.2 70-1072-PRC0054



70-1072-PRC0006

Open-Tray, 3.5 mmP x 3.5 mmD Ø3.7/4.2 70-1072-PRC0006



70-1072-PRC0008

Open-Tray, 3.5 mmP x 4.7 mmD Ø3.7/4.2 70-1072-PRC0008



70-1072-PRC0010

Open-Tray, 4.5 mmP x 4.5 mmD Ø4.7/5.2 70-1072-PRC0010



70-1072-PRC0012

Open-Tray, 4.5 mmP x 5.7 mmD Ø4.7/5.2 70-1072-PRC0012

(Open-Tray Transfer Copings include Open-Tray Screw and Guide Pin.)

INCLUSIVE® TAPERED IMPLANT SCAN BODY



70-1073-PRA0080

3.0 mmP Ø3.2 70-1073-PRA0080



70-1073-PRA0081

3.5 mmP Ø3.7/4.2 70-1073-PRA0081



70-1073-PRA0079

4.5 mmP Ø4.7/5.2 70-1073-PRA0079


(Scan Bodies include captured screw.)

INCLUSIVE® TAPERED IMPLANT ANALOG



70-1072-PRC0055

3.0 mmP Ø3.2 70-1072-PRC0055

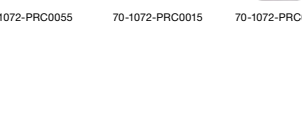

70-1072-PRC0015

3.5 mmP Ø3.7/4.2 70-1072-PRC0015




70-1072-PRC0017

4.5 mmP Ø4.7/5.2 70-1072-PRC0017

STOCK ABUTMENTS

DESCRIPTION IMPLANT CODE

INCLUSIVE® TAPERED IMPLANT 15° TITANIUM ESTHETIC ABUTMENT

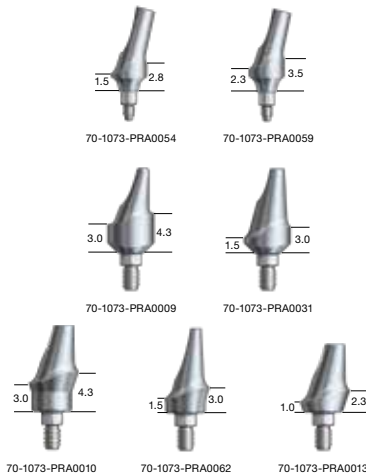

Anterior, 3.0 mmP x 1.5 mmH	Ø3.2	70-1073-PRA0054
Anterior, 3.0 mmP x 2.3 mmH	Ø3.2	70-1073-PRA0059
Anterior, 3.5 mmP	Ø3.7/4.2	70-1073-PRA0009
Anterior, 3.5 mmP x 1.5 mmH.....	Ø3.7/4.2	70-1073-PRA0031
Anterior, 4.5 mmP	Ø4.7/5.2	70-1073-PRA0010
Anterior, 4.5 mmP x 1.5 mmH.....	Ø4.7/5.2	70-1073-PRA0062
Posterior, 4.5 mmP	Ø4.7/5.2	70-1073-PRA0013

INCLUSIVE® TAPERED IMPLANT TITANIUM ESTHETIC ABUTMENT



Anterior, 3.0 mmP x 1.5 mmH	Ø3.2	70-1073-PRA0055
Anterior, 3.0 mmP x 2.3 mmH	Ø3.2	70-1073-PRA0060
Anterior, 3.5 mmP x 1.5 mmH.....	Ø3.7/4.2	70-1073-PRA0032
Anterior, 3.5 mmP	Ø3.7/4.2	70-1073-PRA0011
Anterior, 4.5 mmP	Ø4.7/5.2	70-1073-PRA0012
Anterior, 4.5 mmP x 1.5 mmH.....	Ø4.7/5.2	70-1073-PRA0063
Posterior, 4.5 mmP	Ø4.7/5.2	70-1073-PRA0014
Posterior, Wide, 4.5 mmP.....	Ø4.7/5.2.....	70-1073-PRA0015

(Esthetic Abutments include Titanium Screw.)

INCLUSIVE® TAPERED IMPLANT TITANIUM ABUTMENT



3.0 mmP x 4.5 mmH	Ø3.2	70-1073-PRA0052
3.0 mmP x 6 mmH	Ø3.2	70-1073-PRA0053
3.5 mmP x 4.5 mmH	Ø3.7/4.2	70-1073-PRA0045
3.5 mmP x 6 mmH.....	Ø3.7/4.2	70-1073-PRA0006
4.5 mmP x 4.5 mmH	Ø4.7/5.2	70-1073-PRA0046
4.5 mmP x 6 mmH	Ø4.7/5.2	70-1073-PRA0008

(Titanium Screw sold separately; please see page 9.)



STOCK ABUTMENTS


DESCRIPTION IMPLANT CODE

INCLUSIVE® TAPERED IMPLANT UCLA GOLD ABUTMENT



3.0 mmP.....	Ø3.2.....	70-1073-PRA0056
3.5 mmP.....	Ø3.7/4.2.....	70-1073-PRA0027
4.5 mmP.....	Ø4.7/5.2.....	70-1073-PRA0029

INCLUSIVE® TAPERED IMPLANT UCLA PLASTIC ABUTMENT

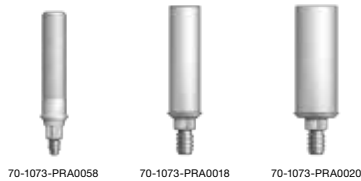

3.0 mmP.....	Ø3.2.....	70-1073-PRA0058
3.5 mmP.....	Ø3.7/4.2.....	70-1073-PRA0018
4.5 mmP.....	Ø4.7/5.2.....	70-1073-PRA0020




Non-Engaging, 3.0 mmP.....	Ø3.2.....	70-1073-PRA0057
Non-Engaging, 3.5 mmP.....	Ø3.7/4.2.....	70-1073-PRA0019
Non-Engaging, 4.5 mmP.....	Ø4.7/5.2.....	70-1073-PRA0021

(UCLA Abutments include Titanium Screw and Guide Pin.)

SCREWS & GUIDE PINS


INCLUSIVE® TAPERED IMPLANT



Titanium Screw 3.0 mmP.....	Ø3.2.....	70-1072-PRC0058
Titanium Screw 3.0 mmP (5-pack).....	Ø3.2.....	70-1072-PRC0057



Titanium Screw 3.5/4.5 mmP.....	Ø3.7/4.2/4.7/5.2.....	70-1072-PRC0001
Titanium Screw 3.5/4.5 mmP (5-pack).....	Ø3.7/4.2/4.7/5.2.....	70-1072-PRC0003



INCLUSIVE® TAPERED IMPLANT

Guide Pin 3.0 mmP (5-pack).....	Ø3.2.....	70-1072-PRC0056
Guide Pin 3.5/4.5 mmP (5-pack).....	Ø3.7/4.2/4.7/5.2.....	70-1072-PRC0002


MULTI-UNIT ABUTMENT SYSTEM

DESCRIPTION IMPLANT CODE

INCLUSIVE® TAPERED IMPLANT MULTI-UNIT ABUTMENT




3.0 mmP x 1.5 mmH.....	Ø3.2.....	70-1074-PRS0040
3.0 mmP x 2.5 mmH.....	Ø3.2.....	70-1074-PRS0041
3.0 mmP x 3.5 mmH.....	Ø3.2.....	70-1074-PRS0042




3.5 mmP x 1 mmH.....	Ø3.7/4.2.....	70-1074-PRS0009
3.5 mmP x 2 mmH.....	Ø3.7/4.2.....	70-1074-PRS0010



3.5 mmP x 3 mmH.....	Ø3.7/4.2.....	70-1074-PRS0065
3.5 mmP x 5 mmH.....	Ø3.7/4.2.....	70-1074-PRS0066




4.5 mmP x 1 mmH.....	Ø4.7/5.2.....	70-1074-PRS0011
4.5 mmP x 2 mmH.....	Ø4.7/5.2.....	70-1074-PRS0012



4.5 mmP x 3 mmH.....	Ø4.7/5.2.....	70-1074-PRS0013
4.5 mmP x 5 mmH.....	Ø4.7/5.2.....	70-1074-PRS0014

(Prosthetic Screw sold separately.)

INCLUSIVE® TAPERED IMPLANT 17° MULTI-UNIT ABUTMENT



3.5 mmP x 2 mmH.....	Ø3.7/4.2.....	70-1074-PRS0001
3.5 mmP x 3 mmH.....	Ø3.7/4.2.....	70-1074-PRS0002



4.5 mmP x 2 mmH.....	Ø4.7/5.2.....	70-1074-PRS0003
4.5 mmP x 3 mmH.....	Ø4.7/5.2.....	70-1074-PRS0004
4.5 mmP x 5 mmH.....	Ø4.7/5.2.....	70-1074-PRS0005














INCLUSIVE® TAPERED IMPLANT 30° MULTI-UNIT ABUTMENT



3.5 mmP x 3 mmH.....	Ø3.7/4.2.....	70-1074-PRS0006
4.5 mmP x 3 mmH.....	Ø4.7/5.2.....	70-1074-PRS0007
4.5 mmP x 5 mmH.....	Ø4.7/5.2.....	70-1074-PRS0008

(Angled Multi-Unit Abutments include Angled Abutment Screw. Prosthetic Screw sold separately; please see page 11.)

MULTI-UNIT ACCESSORIES

	DESCRIPTION	CODE
	INCLUSIVE® MULTI-UNIT	
	Temporary Healing Cap with Prosthetic Screw .050" Hex.....	70-1074-PRS0015
<small>70-1074-PRS0015</small>		
	Coping 4.5 mmH, Non-Engaging, with Prosthetic Screw .050" Hex.....	70-1073-PRA0037
<small>70-1073-PRA0037</small>		
	Gold/Plastic Coping.....	70-1074-PRS0030
<small>70-1074-PRS0030</small>		
	Gold Bar Coping	70-1074-PRS0018
<small>70-1074-PRS0018</small>		
	Impression Coping, Open-Tray, with Guide Pin .050" Hex	70-1074-PRS0052
<small>70-1074-PRS0052</small>		
	Impression Coping, Closed-Tray	70-1074-PRS0021
<small>70-1074-PRS0021</small>		
	Titanium Temporary with Prosthetic Screw .050" Hex	70-1074-PRS0025
<small>70-1074-PRS0025</small>		
	Plastic Coping with Prosthetic Screw .050" Hex	70-1074-PRS0067
<small>70-1074-PRS0067</small>		
	Abutment Analog	70-1074-PRS0016
<small>70-1074-PRS0016</small>		
	Driver.....	70-1074-PRS0028
<small>70-1074-PRS0028</small>		
	Guide Pin .050" Hex.....	70-1074-PRS0061
<small>70-1074-PRS0061</small>		
	Prosthetic Screw .050" Hex.....	70-1072-PRC0014
<small>70-1072-PRC0014</small>		
	Inclusive® Angled Multi-Unit Abutment Screw.....	70-1074-PRS0031
<small>70-1074-PRS0031</small>		

LOCATOR® ABUTMENT SYSTEM

	DESCRIPTION	IMPLANT	CODE
	LOCATOR® ABUTMENT 3.0 mmP x 1 mmH Cuff [#2212]].....	Ø3.2.....	70-1075-ZST0065
70-1075-ZST0065			
	3.0 mmP x 3 mmH Cuff [#2214].....	Ø3.2.....	70-1075-ZST0066
70-1075-ZST0066			
	3.5 mmP x 0 mmH Cuff [#8661].....	Ø3.7/4.2.....	70-1075-ZST0011
70-1075-ZST0011			
	3.5 mmP x 1 mmH Cuff [#8662]	Ø3.7/4.2.....	70-1075-ZST0012
70-1075-ZST0012			
	3.5 mmP x 2.5 mmH Cuff [#8663]	Ø3.7/4.2.....	70-1075-ZST0013
70-1075-ZST0013			
	3.5 mmP x 3.5 mmH Cuff [#8664]	Ø3.7/4.2.....	70-1075-ZST0014
70-1075-ZST0014			
	4.5 mmP x 0 mmH Cuff [#8671].....	Ø4.7/5.2.....	70-1075-ZST0015
70-1075-ZST0015			
	4.5 mmP x 1 mmH Cuff [#8672].....	Ø4.7/5.2.....	70-1075-ZST0016
70-1075-ZST0016			
	4.5 mmP x 2 mmH Cuff [#8673].....	Ø4.7/5.2.....	70-1075-ZST0017
70-1075-ZST0017			
	4.5 mmP x 3 mmH Cuff [#8674].....	Ø4.7/5.2.....	70-1075-ZST0018
70-1075-ZST0018			
	4.5 mmP x 4 mmH Cuff [#8675].....	Ø4.7/5.2.....	70-1075-ZST0019
70-1075-ZST0019			

LOCATOR Abutment System available for US market only.

LOCATOR is a registered trademark of Zest Anchors, LLC.

LOCATOR® ACCESSORIES

DESCRIPTION

CODE

LOCATOR® ABUTMENT ACCESSORIES



70-1075-ZST0024

Male Processing Package (2-pack) [#8519-2] 70-1075-ZST0024
(Includes: Denture Cap with Black Processing Male, Clear Nylon Male (5 lbs), Pink (LR) Less-Retentive Nylon Male (3 lbs), Blue Extra-Light-Retention Nylon Male (1.5 lbs), and White Block-out Spacer.)



70-1075-ZST0025

Extended Range Male Processing Package (2-pack) [#8540-2]..... 70-1075-ZST0025
(Includes: Denture Cap with Black Processing Male, Extended-Range Replacement Males: Green (3-4 lbs), Orange (2 lbs), Red (0.5-1.5 lbs), and White Block-Out Spacer.)



70-1075-ZST0007

Impression Coping (4-pack) [#8505] 70-1075-ZST0007



70-1075-ZST0009

Female Analog 4 mmD (4-pack) [#8530] 70-1075-ZST0009



70-1075-ZST0005

Core Tool Abutment Holder Sleeve (4-pack) [#8394] 70-1075-ZST0005



70-1075-ZST0026

Angle Measurement Guide [#9530] 70-1075-ZST0026



70-1075-ZST0010

Processing Spacer (4-pack) [#8569] 70-1075-ZST0010



70-1075-ZST0004

Core Tool (Complete) [#8393] 70-1075-ZST0004



70-1075-ZST0006

Core Tool Male Removal (Tip End) [#8397] 70-1075-ZST0006



70-1075-ZST0008

Parallel Post (4-pack) [#8517] 70-1075-ZST0008



70-1075-ZST0003

Core Tool Abutment Driver (Gold End) [#8390] 70-1075-ZST0003




70-1075-ZST0001

35 Ncm Torque Wrench Insert Driver (15 mm) [#8260]..... 70-1075-ZST0001



70-1075-ZST0002

35 Ncm Torque Wrench Insert Driver (21 mm) [#8280] 70-1075-ZST0002



70-1075-ZST0020

Latch Type Torque Wrench Insert Driver (23 mm) [#8913] 70-1075-ZST0020



70-1075-ZST0021

Latch Type Torque Wrench Insert Driver (29 mm) [#8914] 70-1075-ZST0021



70-1075-ZST0022

Square Drive Torque Wrench Insert Driver (15 mm) [#8926] 70-1075-ZST0022



70-1075-ZST0023

Square Drive Torque Wrench Insert Driver (21 mm) [#8927] 70-1075-ZST0023


SURGICAL KIT



DESCRIPTION

CODE

Inclusive® Tapered Implant Surgical Instrumentation Kit70-1071-IMP002

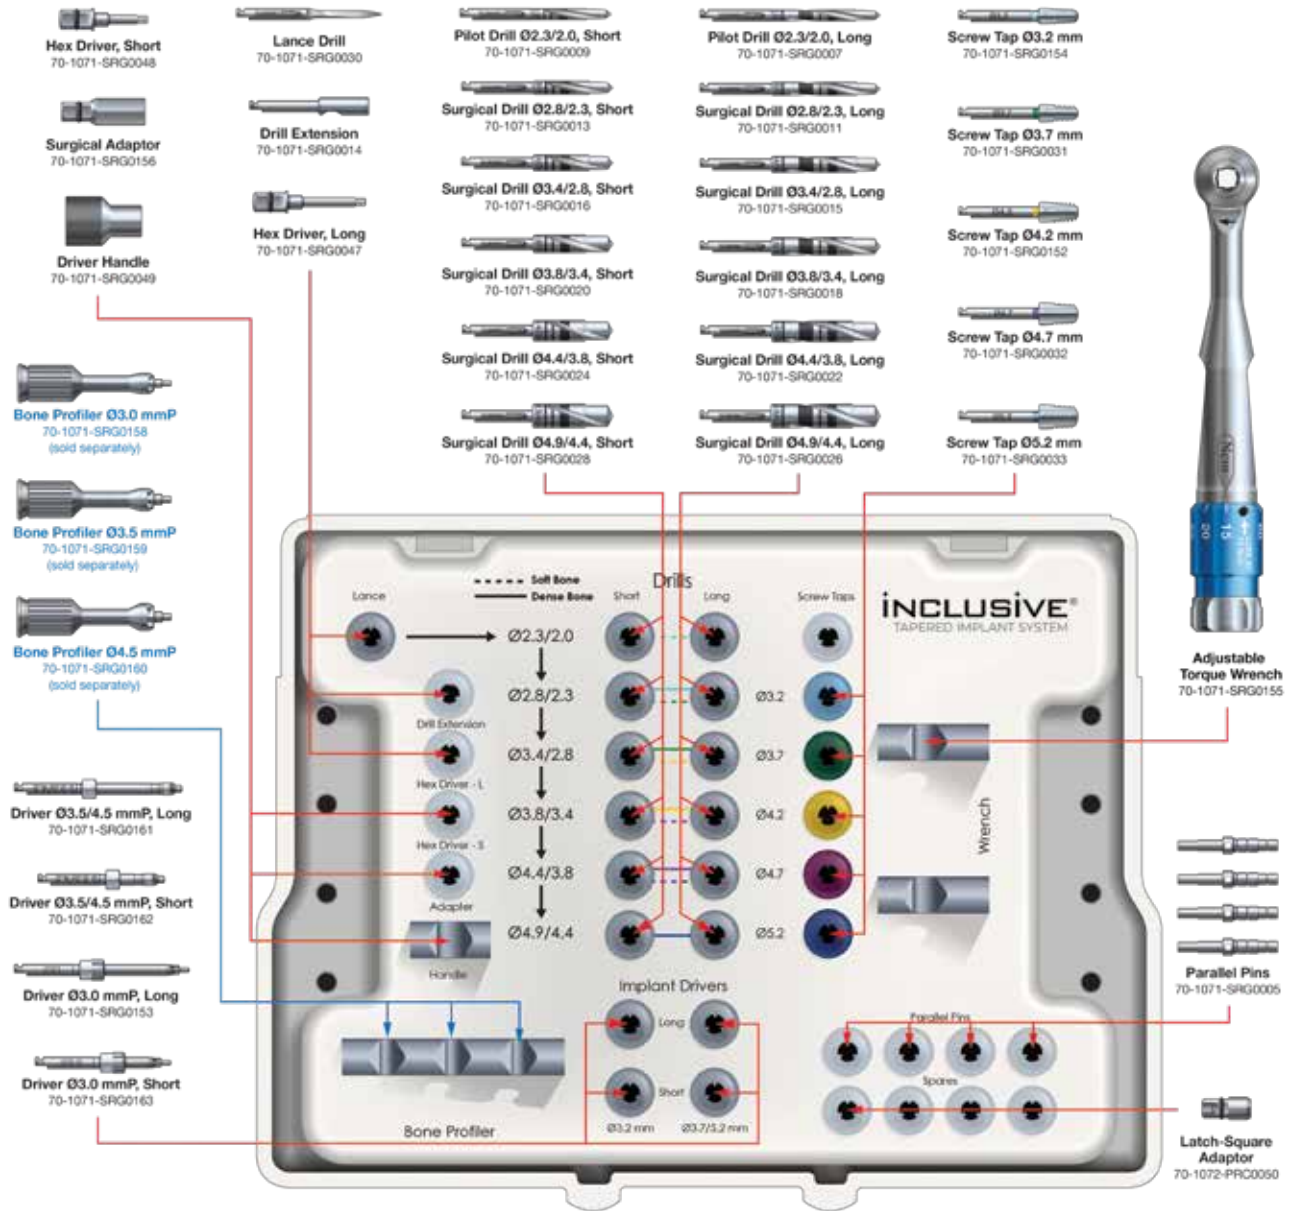

(Bone Profilers sold separately)


PROSTHETIC KIT



DESCRIPTION

CODE

Inclusive® Tapered Implant Prosthetic Kit..... 70-1071-PRS0001

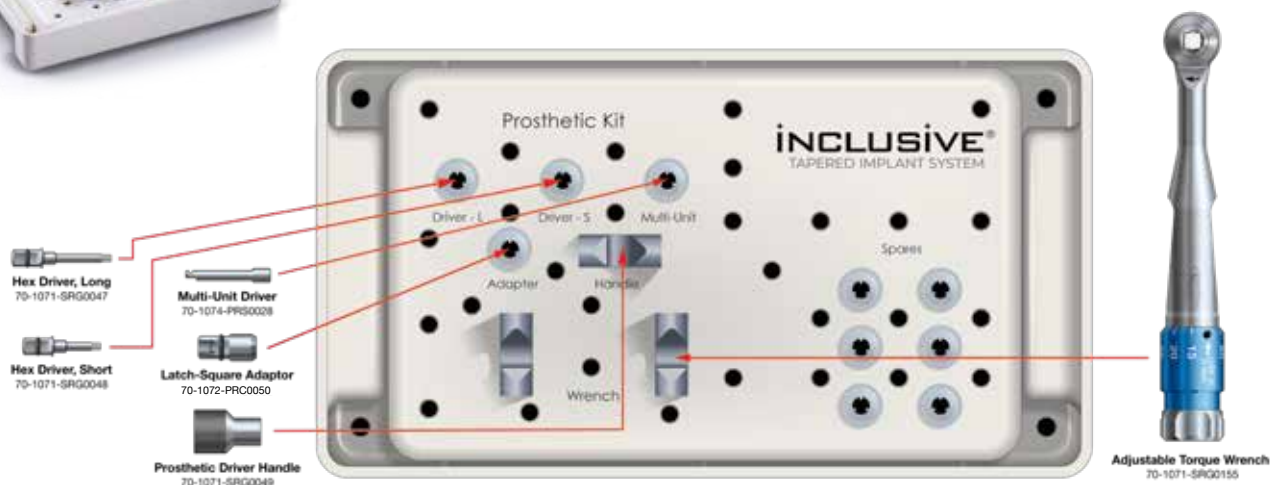

FEATURES AND BENEFITS

The instrumentation kits allow the clinician to easily organize, store and transport the surgical and prosthetic tooling of the Inclusive Tapered Implant System. The autoclavable kits have been designed for ease of use, with component labels for identification.

The color-coded surgical kit clearly maps the drilling protocol for each implant. Drills are arranged from top to bottom in order of increasing diameter, with color-coded fields to indicate the corresponding diameter of Inclusive Tapered Implant for both soft bone and dense bone protocols. **Please note that Bone Profilers are sold separately (refer to diagram, page 17).**

The prosthetic kit is designed specifically for restorative doctors, organizing all of the necessary prosthetic tooling to help simplify restorative procedures and instrument sterilization.

All instruments associated with the Inclusive Tapered Implant System are machined from corrosion-resistant, surgical stainless steel, and feature standard connectivity. All instrumentation is manufactured in the USA or Switzerland. For specific country of origin, please refer to the individual product label.

STERILITY

Surgical instruments are shipped non-sterile. Surgical tray and instruments must be cleaned, disinfected, and sterilized prior to clinical use, according to a validated method.

■ **Cleaning:** Wash using a broad spectrum cleaning solution, followed by thorough rinsing and drying. The recommended disinfection process is based on ANSI/AAMI ST79 guidelines, as follows:

■ **Disinfection:** Immerse in disinfectant¹, rinse with distilled water and dry. The recommended sterilization process is based on the ANSI/AAMI/ISO 17665-1 and ANSI/AAMI ST79 guidelines, as follows:

■ **Sterilization:** Gravity-fed sterilizers: Autoclave is sterilization pouch for 15 minutes at 132°C (270°F). Allow sterilized components to dry for at least 30 minutes.





NOTE: The validated procedures require the use of FDA-cleared sterilization trays, wraps, biological indicators, chemical indicators, and other sterilization accessories labeled for the sterilization cycle recommended. The healthcare facility should monitor the sterilizer for the facility according to an FDA-recognized sterility assurance standard such as ANSI/AAMI ST79.

GENERAL CLEANING TIPS:

- Observe universal precautions for the handling of contaminated or biohazardous materials.
- Clean promptly after each use, to prevent biological fluids and tissues from drying on the instruments.
- When applicable, disassemble parts and instruments prior to cleaning.
- Do not rely solely on automatic cleaning. Thorough manual cleaning is recommended.

¹ Oral disinfectant containing *Chlorhexidine* is recommended; refer to the disinfectant manufacturer's instructions.

DRILLS & TAPS

	DESCRIPTION	CODE
INCLUSIVE®		
 70-1071-SRG0030	Lance Drill Ø1.5 mm	70-1071-SRG0030
 70-1071-SRG0007	Pilot Drill Ø2.3/2.0 mm, Long.....	70-1071-SRG0007
 70-1071-SRG0009	Pilot Drill Ø2.3/2.0 mm, Short.....	70-1071-SRG0009
 70-1071-SRG0011	Surgical Drill Ø2.8/2.3 mm, Long	70-1071-SRG0011
 70-1071-SRG0013	Surgical Drill Ø2.8/2.3 mm, Short.....	70-1071-SRG0013
 70-1071-SRG0015	Surgical Drill Ø3.4/2.8 mm, Long	70-1071-SRG0015
 70-1071-SRG0016	Surgical Drill Ø3.4/2.8 mm, Shortt	70-1071-SRG0016
 70-1071-SRG0018	Surgical Drill Ø3.8/3.4 mm, Long	70-1071-SRG0018
 70-1071-SRG0020	Surgical Drill Ø3.8/3.4 mm, Short	70-1071-SRG0020
 70-1071-SRG0022	Surgical Drill Ø4.4/3.8 mm, Long	70-1071-SRG0022
 70-1071-SRG0024	Surgical Drill Ø4.4/3.8 mm, Short	70-1071-SRG0024
 70-1071-SRG0026	Surgical Drill Ø4.9/4.4 mm, Long	70-1071-SRG0026
 70-1071-SRG0028	Surgical Drill Ø4.9/4.4 mm, Short.....	70-1071-SRG0028
 70-1071-SRG0154	Screw Tap Ø3.2 mm	70-1071-SRG0154
 70-1071-SRG0031	Screw Tap Ø3.7 mm	70-1071-SRG0031
 70-1071-SRG0152	Screw Tap Ø4.2 mm	70-1071-SRG0152
 70-1071-SRG0032	Screw Tap Ø4.7 mm	70-1071-SRG0032
 70-1071-SRG0033	Screw Tap Ø5.2 mm	70-1071-SRG0033

INSTRUMENTATION


	DESCRIPTION	CODE
 <small>70-1071-SRG0158</small>	Inclusive® Bone Profiler Ø3.0 mmP	70-1071-SRG0158
 <small>70-1071-SRG0159</small>	Inclusive® Bone Profiler Ø3.5 mmP	70-1071-SRG0159
 <small>70-1071-SRG0160</small>	Inclusive® Bone Profiler Ø4.5 mmP	70-1071-SRG0160
 <small>70-1071-SRG0153</small>	Inclusive® Tapered Implant Driver Ø3.0 mmP, Long	70-1071-SRG0153
 <small>70-1071-SRG0163</small>	Inclusive® Tapered Implant Driver Ø3.0 mmP, Short.....	70-1071-SRG0163
 <small>70-1071-SRG0161</small>	Inclusive® Tapered Implant Driver Ø3.5/4.5 mmP, Long	70-1071-SRG0161
 <small>70-1071-SRG0162</small>	Inclusive® Tapered Implant Driver Ø3.5/4.5 mmP, Short.....	70-1071-SRG0162
 <small>70-1071-SRG0047</small>	Inclusive® Prosthetic Driver .050" Hex, Long	70-1071-SRG0047
 <small>70-1071-SRG0048</small>	Inclusive® Prosthetic Driver .050" Hex, Short	70-1071-SRG0048
 <small>70-1071-SRG0155</small>	Adjustable Torque Wrench	70-1071-SRG0155
 <small>70-45721-401</small>	Torque Wrench.....	70-45721-401
 <small>70-1071-SRG0157</small>	Ratchet Wrench	70-1071-SRG0157
 <small>70-1071-SRG0005</small>	Inclusive® Parallel Pin.....	70-1071-SRG0005
 <small>70-1071-SRG0014</small>	Inclusive® Drill Extender.....	70-1071-SRG0014
 <small>70-1071-SRG0049</small>	Inclusive® Driver Handle	70-1071-SRG0049
 <small>70-1072-PRC0050</small>	Inclusive® Latch-Square Adaptor	70-1072-PRC0050
 <small>70-1071-SRG0156</small>	Inclusive® Tapered Implant Surgical Adaptor.....	70-1071-SRG0156
 <small>70-1071-IMP0001</small>	Inclusive® Tapered Implant Radiographic Template	70-1071-IMP0001

INCLUSIVE® MINI IMPLANT TECHNICAL SPECIFICATIONS

Below is an enhanced view of the Inclusive Mini Implant with O-ball Head prosthetic attachment, including a side-by-side comparison of the 2.2 mm diameter, 2.5 mm diameter, and 3.0 mm diameter implants. The stated length (10 mm, 13 mm, or 15 mm) refers to the thread length (endosseous section) of the implant, which includes the micro-threaded base of the transgingival collar.

INCLUSIVE®

MINI IMPLANT SYSTEM

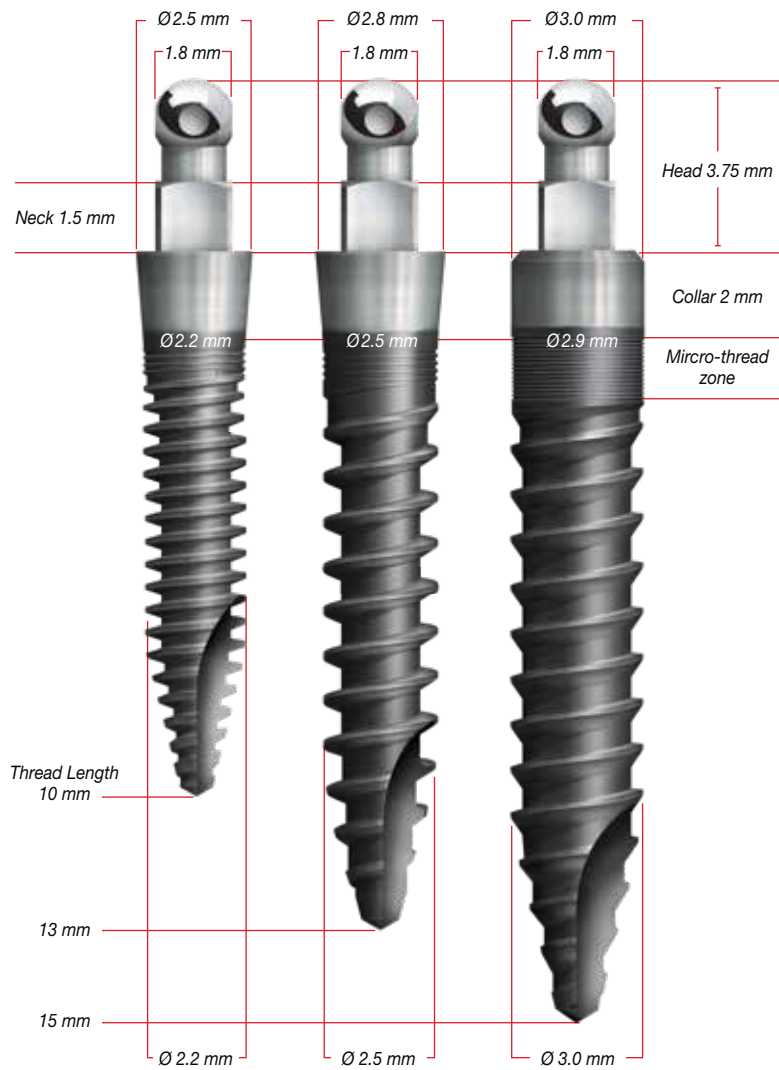

MINI IMPLANTS

Inclusive Mini Implants are self-tapping threaded titanium implants designed for provisional and long-term applications. These devices will allow immediate loading and long-term stabilization of dentures and provisional stabilization of dentures while standard implants heal. The implants are to be used for immediate loading only in the presence of primary stability and appropriate occlusal loading.

DESCRIPTION _____ CODE _____



70-1068-IMP0001



70-1068-IMP0002



70-1068-IMP0003

INCLUSIVE® MINI IMPLANT O-BALL

2.2 mmD x 10 mmL.....	70-1068-IMP0001
2.2 mmD x 13 mmL.....	70-1068-IMP0002
2.2 mmD x 15 mmL.....	70-1068-IMP0003



70-1068-IMP0004



70-1068-IMP0005



70-1068-IMP0006

2.5 mmD x 10 mmL.....	70-1068-IMP0004
2.5 mmD x 13 mmL.....	70-1068-IMP0005
2.5 mmD x 15 mmL.....	70-1068-IMP0006



70-1068-IMP0007



70-1068-IMP0008




70-1068-IMP0009

3.0 mmD x 10 mmL.....	70-1068-IMP0007
3.0 mmD x 13 mmL.....	70-1068-IMP0008
3.0 mmD x 15 mmL.....	70-1068-IMP0009

INCLUSIVE® MINI IMPLANT PROSTHETIC COMPONENTS

The O-ring Housing serves as the retention cap for each Inclusive Mini Implant that is placed. The housing is picked up by the patient's prosthesis using a hard reline of the new or existing denture. These loading procedures can typically be performed immediately after placement of the Inclusive Mini Implants, provided primary stability and appropriate occlusal loading are assured.

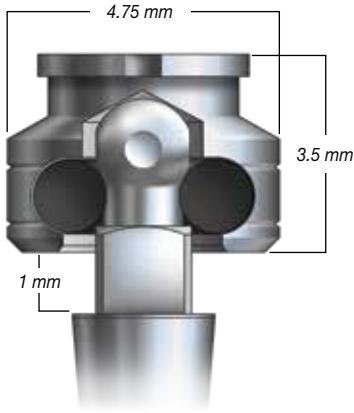

The housing is 3.5 mm in height, and 4.75 mm in diameter. The same housing is used regardless of the diameter or length of the selected Inclusive Mini Implant. A vertical space of approximately 1 mm between the crest of the implant collar and the mouth of the housing provides for up to 30 degrees of angular divergence between seated implants.

Each housing comes packaged with one 3/16" x 1/16" O-ring seated within, plus one extra replacement O-ring.

DESCRIPTION _____ CODE _____



INCLUSIVE® MINI IMPLANT
O-Ring Housing 70-1066-MNP0006



Prosthetic O-Rings 3/16" x 1/16" (10-pack)..... 70-1066-MNP0008



Blockout Shims (25-pack)..... 70-1066-MNI0001



Impression Coping (4-pack) 70-1066-MNP0004




Replica (4-pack) 70-1066-MNP0005



Instrumentation O-Rings 2.5 mm x 1 mm (5-pack)..... 70-1066-MNP0007

INCLUSIVE® MINI IMPLANT SURGICAL KIT OVERVIEW

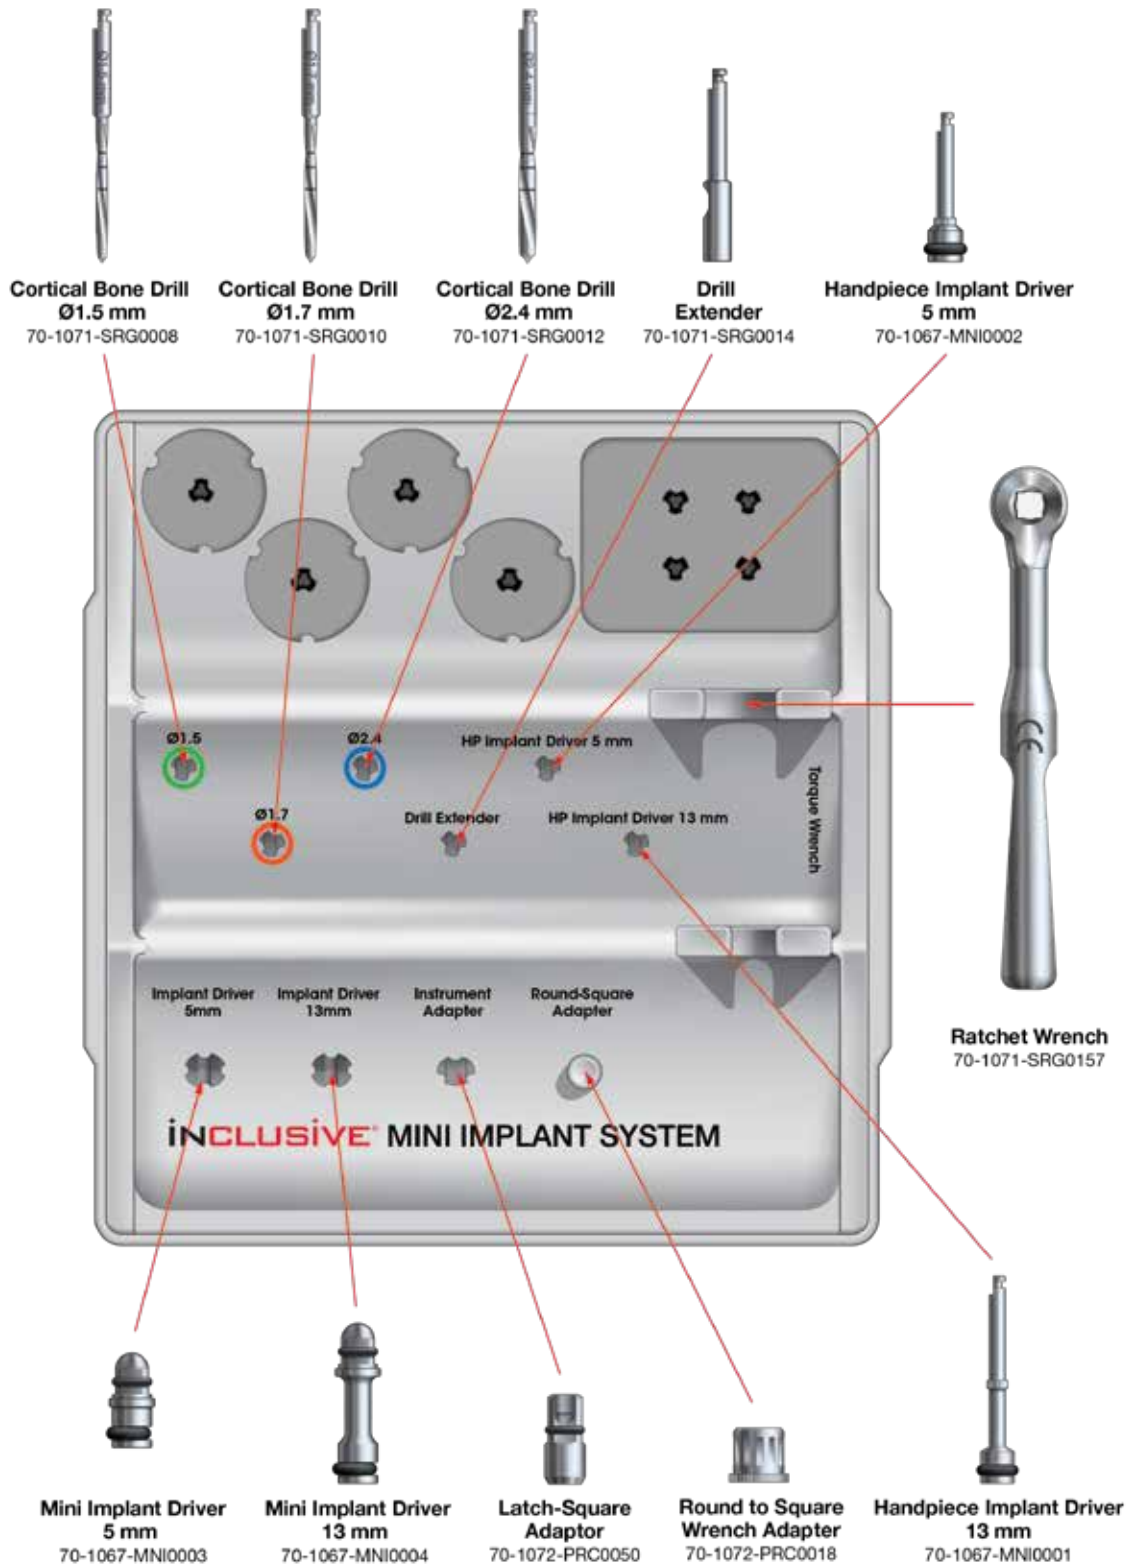

INCLUSIVE® MINI IMPLANT SURGICAL KIT

All instruments associated with the Inclusive Mini Implant system are machined from high-quality, corrosion-resistant, surgical stainless steel.



DESCRIPTION	CODE
Inclusive® Mini Implant Surgical Instrumentation Kit.....	70-1067-MNI0006

FEATURES AND BENEFITS

The Mini Implant Surgical Instrumentation Kit allows the clinician to easily organize, store and transport the components of the Inclusive Mini Implant System. It has been designed for ease of use, with component markings and angled rows for easy identification and to help maximize space. The durable, synthetic material is autoclavable and provides a snug, secure fit.

Drills are arranged from left to right in order of increasing diameter, with color-coded fields to indicate the corresponding diameter of Inclusive Mini Implant.

STERILITY

Surgical instruments are shipped non-sterile. Surgical tray and instruments must be cleaned, disinfected, and sterilized prior to clinical use, according to a validated method.

- **Cleaning:** Wash using a broad spectrum cleaning solution, followed by thorough rinsing and drying. The recommended disinfection process is based on ANSI/AAMI ST79 guidelines, as follows:
- **Disinfection:** Immerse in disinfectant¹, rinse with distilled water and dry. The recommended sterilization process is based on the ANSI/AAMI/ISO 17665-1 and ANSI/AAMI ST79 guidelines, as follows:
- **Sterilization:** Gravity-fed sterilizers: Autoclave in sterilization pouch for 20 minutes at 132°C (270°F). Devices are to be used immediately after sterilization.



NOTE: The validated procedures require the use of FDA-cleared sterilization trays, wraps, biological indicators, chemical indicators, and other sterilization accessories labeled for the sterilization cycle recommended. The healthcare facility should monitor the sterilizer for the facility according to an FDA-recognized sterility assurance standard such as ANSI/AAMI ST79.

¹ Oral disinfectant containing *Chlorhexidine* is recommended; refer to the disinfectant manufacturer's instructions.

GENERAL CLEANING TIPS:

- Observe universal precautions for the handling of contaminated or biohazardous materials.
- Clean promptly after each use, to prevent biological fluids and tissues from drying on the instruments.
- When applicable, disassemble parts and instruments prior to cleaning.
- Do not rely solely on automatic cleaning. Thorough manual cleaning is recommended.

INCLUSIVE® MINI IMPLANT INSTRUMENTATION

	DESCRIPTION	CODE
 <small>70-1071-SRG0008</small>	Inclusive® Cortical Bone Drill Ø1.5 mm	70-1071-SRG0008
 <small>70-1071-SRG0010</small>	Inclusive® Cortical Bone Drill Ø1.7 mm	70-1071-SRG0010
 <small>70-1071-SRG0012</small>	Inclusive® Cortical Bone Drill Ø2.4 mm	70-1071-SRG0012
 <small>70-1071-SRG0014</small>	Inclusive® Drill Extender.....	70-1071-SRG0014
 <small>70-1067-MNI0004</small>	Inclusive® Mini Implant Driver 13 mm	70-1067-MNI0004
 <small>70-1067-MNI0003</small>	Inclusive® Mini Implant Driver 5 mm.....	70-1067-MNI0003
 <small>70-1067-MNI0001</small>	Inclusive® Handpiece Mini Implant Driver 13 mm	70-1067-MNI0001
 <small>70-1067-MNI0002</small>	Inclusive® Handpiece Mini Implant Driver 5 mm	70-1067-MNI0002
 <small>70-1071-SRG0157</small>	Ratchet Wrench	70-1071-SRG0157
 <small>70-1072-PRC0050</small>	Inclusive® Latch-Square Adaptor	70-1072-PRC0050
 <small>70-1067-MNI0007</small>	Inclusive® Mini Implant Radiographic Template.....	70-1067-MNI0007

IMPLANT PACKAGING

Inclusive Implants are shipped sterile, and should not be resterilized. They are for single-use only, prior to the expiration date. Do not use implants if packaging has been compromised or previously opened. Do not handle implant surfaces directly. Users are advised to visually inspect packaging to ensure seals and contents are intact prior to use. Please refer to the individual product label for all relevant product information and cautions.

EXPLANATION OF LABEL CODES:

1. Official product description
2. Date of Manufacture (YYYY-MM-DD)
3. Catalog Number
4. Lot/Batch Number
5. By Prescription Only
6. Do Not Use if Package is Damaged
7. Sterile with Gamma Radiation
8. Use-by Date
9. Consult Instructions for Use
10. Do not Re-use
11. Do not Resterilize
12. Manufacturer
13. Country of origin
14. Unique Device Identification (UDI)
15. QR code for IFU website



4.2 mmD x 13 mmL	<p>1 Inclusive® Tapered Implant 4.2 mmD x 13 mmL x 3.5 mmP</p> <p>7 STERILE R 8 Use by YYYY-MM-DD 11 9 </p> <p>6 Do not use if package is damaged. 10 </p> <p>12 Prisma^{ti}k Dentalcraft, Inc. 2144 Michelson Drive Irvine, CA 92612, USA YYYY-MM-DD 2 Made in USA 13 14 </p> <p>4 LOT 1234567 1 pc. </p> <p>https://ifu.glidewelldental.com IFU CODE: IFU-012570 tel: (888) 402-1725</p> <p>5 Scan QR code for link to URL For more information email mail@glidewelldental.com 15 </p> <p>3031898_8.0</p>	4.2 mmD x 13 mmL
4.2 mmD x 13 mmL	<p>3 REF 70-1070-IMP0029 INCLUSIVE®</p>	

POLICIES AND WARRANTY

ORDERING INFORMATION

In the U.S.: Order at glidewelldirect.com or call Glidewell Direct at 888-303-3975. Our product specialists are committed to answering questions in a timely fashion to ensure your ordering is easy and efficient. We are available Monday—Friday from 6 a.m.—5 p.m. (*Pacific*).

In Canada: Call 888-278-0414 to order. All others: Please send inquiries to: international@glidewelldirect.com.

SHIPPING POLICY

- Orders placed after 3 p.m. (*Pacific*) will be processed on the following business day. Business days do not include Saturdays, Sundays, or U.S. holidays.
- Online shopping cart available to U.S. customers only.

TERMS

All accounts are payable within 30 days of invoice date. Accounts not paid within the stated terms will be subject to COD status and a late charge of 2 percent of the unpaid balance. We accept American Express, Visa, MasterCard, and Discover. All prices are subject to change without notice.

PRODUCT RETURN POLICY

Products may be returned at the customer's expense for credit within 30 days of invoice date. All returned products must meet the following conditions:

- A copy of the original invoice must accompany the products.
- Products must be packaged to arrive at the seller's facility undamaged.
- Discontinued, obsolete, expired, damaged, or opened items will not be accepted for return.
- Amount credited will be based on invoice price, less 15 percent for restocking fee.
- Shipping charges are the responsibility of the customer and will not be credited.

PRODUCT & PRICING CHANGES

Because products and equipment are continually undergoing refinement in design and manufacturing methods, we reserve the right to improve, modify, or discontinue products and equipment or change pricing at any time without incurring any obligation and without prior notice.

WARRANTY

Limited Warranty—Prismatik Dentalcraft, Inc.

Prismatik Dentalcraft, Inc. ("Prismatik"), is the manufacturer of dental products (the "product"), including Inclusive® Dental Implants ("implants"). Prismatik and Glidewell Direct hereinafter are referred to collectively as Glidewell. For a period from the original purchase date of seven (7) years for implants and six (6) months for ceramic blanks and any other product ("the warranty period"), Glidewell will at its option replace or refund the purchase price of any product, to the original purchaser ("user"), that is returned due to defects in material and manufacture.

NO GUARANTEE OR WARRANTY IS IMPLIED OTHER THAN EXPRESSLY STATED, INCLUDING ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.

Glidewell shall not be liable for any incidental or consequential damages, whether foreseeable or not, caused by defects in the product or dental devices produced using said product. User is responsible for determining the suitability of the product for user's application. If this product is defective within the warranty period, user's exclusive remedy and Glidewell's sole obligation shall be replacement or refund of the purchase price of the product. For replacement or refund under this warranty, the original purchaser shall send the product at its own expense, postage prepaid, to Glidewell Direct, 18651 Von Karman Ave, Irvine, CA 92612.

PARTS INDEX

CODE DESCRIPTION PAGE

INCLUSIVE TAPERED IMPLANT SYSTEM

IMPLANTS

70-1070-IMP0036.....	Tapered Implant 3.2 mmD x 10 mmL.....	5
70-1070-IMP0032.....	Tapered Implant 3.2 mmD x 11.5 mmL.....	5
70-1070-IMP0033.....	Tapered Implant 3.2 mmD x 13 mmL.....	5
70-1070-IMP0034.....	Tapered Implant 3.2 mmD x 16 mmL.....	5
70-1070-IMP0035.....	Tapered Implant 3.2 mmD x 8 mmL.....	5
70-1070-IMP0006.....	Tapered Implant 3.7 mmD x 10 mmL.....	5
70-1070-IMP0007.....	Tapered Implant 3.7 mmD x 11.5 mmL.....	5
70-1070-IMP0008.....	Tapered Implant 3.7 mmD x 13 mmL.....	5
70-1070-IMP0009.....	Tapered Implant 3.7 mmD x 16 mmL.....	5
70-1070-IMP0005.....	Tapered Implant 3.7 mmD x 8 mmL.....	5
70-1070-IMP0027.....	Tapered Implant 4.2 mmD x 10 mmL.....	5
70-1070-IMP0028.....	Tapered Implant 4.2 mmD x 11.5 mmL.....	5
70-1070-IMP0029.....	Tapered Implant 4.2 mmD x 13 mmL.....	5
70-1070-IMP0030.....	Tapered Implant 4.2 mmD x 16 mmL.....	5
70-1070-IMP0026.....	Tapered Implant 4.2 mmD x 8 mmL.....	5
70-1070-IMP0011.....	Tapered Implant 4.7 mmD x 10 mmL.....	5
70-1070-IMP0012.....	Tapered Implant 4.7 mmD x 11.5 mmL.....	5
70-1070-IMP0013.....	Tapered Implant 4.7 mmD x 13 mmL.....	5
70-1070-IMP0014.....	Tapered Implant 4.7 mmD x 16 mmL.....	5
70-1070-IMP0010.....	Tapered Implant 4.7 mmD x 8 mmL.....	5
70-1070-IMP0016.....	Tapered Implant 5.2 mmD x 10 mmL.....	5
70-1070-IMP0017.....	Tapered Implant 5.2 mmD x 11.5 mmL.....	5
70-1070-IMP0018.....	Tapered Implant 5.2 mmD x 13 mmL.....	5
70-1070-IMP0019.....	Tapered Implant 5.2 mmD x 16 mmL.....	5
70-1070-IMP0015.....	Tapered Implant 5.2 mmD x 8 mmL.....	5

INSTRUMENTATION

70-1071-PRS0001.....	Prosthetic Kit.....	15
70-1071-IMP0002.....	Surgical Instrumentation Kit.....	14

INSTRUMENTATION - DRILLS & TAPS

70-1071-SRG0030.....	Lance Drill Ø1.5 mm.....	16
70-1071-SRG0007.....	Pilot Drill Ø2.3/2.0 mm, Long.....	16
70-1071-SRG0009.....	Pilot Drill Ø2.3/2.0 mm, Short.....	16
70-1071-SRG0154.....	Screw Tap Ø3.2 mm.....	16
70-1071-SRG0031.....	Screw Tap Ø3.7 mm.....	16
70-1071-SRG0152.....	Screw Tap Ø4.2 mm.....	16
70-1071-SRG0032.....	Screw Tap Ø4.7 mm.....	16
70-1071-SRG0033.....	Screw Tap Ø5.2 mm.....	16
70-1071-SRG0011.....	Surgical Drill Ø2.8/2.3 mm, Long.....	16
70-1071-SRG0013.....	Surgical Drill Ø2.8/2.3 mm, Short.....	16
70-1071-SRG0015.....	Surgical Drill Ø3.4/2.8 mm, Long.....	16
70-1071-SRG0016.....	Surgical Drill Ø3.4/2.8 mm, Short.....	16
70-1071-SRG0018.....	Surgical Drill Ø3.8/3.4 mm, Long.....	16
70-1071-SRG0020.....	Surgical Drill Ø3.8/3.4 mm, Short.....	16
70-1071-SRG0022.....	Surgical Drill Ø4.4/3.8 mm, Long.....	16
70-1071-SRG0024.....	Surgical Drill Ø4.4/3.8 mm, Short.....	16
70-1071-SRG0026.....	Surgical Drill Ø4.9/4.4 mm, Long.....	16
70-1071-SRG0028.....	Surgical Drill Ø4.9/4.4 mm, Short.....	16

INSTRUMENTATION - DRIVERS & ACCESSORIES

70-1071-SRG0155.....	Adjustable Torque Wrench.....	17
70-1071-SRG0158.....	Bone Profiler Ø3.0.....	17
70-1071-SRG0159.....	Bone Profiler Ø3.5.....	17
70-1071-SRG0160.....	Bone Profiler Ø4.5.....	17
70-1071-SRG0014.....	Drill Extender.....	17,23
70-1071-SRG0049.....	Driver Handle.....	17
70-1071-SRG0153.....	Implant Driver Ø3.2 Long.....	17
70-1072-PRC0050.....	Latch-Square Adaptor.....	17,23
70-1071-SRG0005.....	Parallel Pin.....	17
70-1071-SRG0047.....	Prosthetic Driver .050" Hex, Long.....	17
70-1071-SRG0048.....	Prosthetic Driver .050" Hex, Short.....	17
70-1071-IMP0001.....	Radiographic Template.....	17
70-1071-SRG0157.....	Ratchet Wrench.....	17,23

CODE DESCRIPTION PAGE

70-1071-SRG0156.....	Surgical Adaptor.....	17
70-1071-SRG0163.....	Tapered Implant Driver Ø3.0 mmP, Short.....	17
70-1071-SRG0161.....	Tapered Implant Driver Ø3.5/4.5 mmP, Long.....	17
70-1071-SRG0162.....	Tapered Implant Driver Ø3.5/4.5 mmP, Short.....	17
70-45721-401.....	Torque Wrench.....	17

PROSTHETICS - HEALING/TEMPORIZATION

70-1069-IMP0009.....	Healing Abutment 3.0 mmP x 3.2 mmD x 3 mmH.....	6
70-1069-IMP0010.....	Healing Abutment 3.0 mmP x 3.2 mmD x 5 mmH.....	6
70-1069-IMP0011.....	Healing Abutment 3.0 mmP x 3.2 mmD x 7 mmH.....	6
70-1069-IMP0012.....	Healing Abutment 3.0 mmP x 3.7 mmD x 3 mmH.....	6
70-1069-IMP0013.....	Healing Abutment 3.0 mmP x 3.7 mmD x 5 mmH.....	6
70-1069-IMP0014.....	Healing Abutment 3.0 mmP x 3.7 mmD x 7 mmH.....	6
70-1069-IMP0001.....	Healing Abutment 3.5 mmP x 3.5 mmD x 3 mmH.....	6
70-1069-IMP0002.....	Healing Abutment 3.5 mmP x 3.5 mmD x 5 mmH.....	6
70-1069-IMP0015.....	Healing Abutment 3.5 mmP x 3.5 mmD x 7 mmH.....	6
70-1069-IMP0003.....	Healing Abutment 3.5 mmP x 4.7 mmD x 3 mmH.....	6
70-1069-IMP0004.....	Healing Abutment 3.5 mmP x 4.7 mmD x 5 mmH.....	6
70-1069-IMP0016.....	Healing Abutment 3.5 mmP x 4.7 mmD x 7 mmH.....	6
70-1069-IMP0005.....	Healing Abutment 4.5 mmP x 4.5 mmD x 3 mmH.....	6
70-1069-IMP0006.....	Healing Abutment 4.5 mmP x 4.5 mmD x 5 mmH.....	6
70-1069-IMP0017.....	Healing Abutment 4.5 mmP x 4.5 mmD x 7 mmH.....	6
70-1069-IMP0007.....	Healing Abutment 4.5 mmP x 5.7 mmD x 3 mmH.....	6
70-1069-IMP0008.....	Healing Abutment 4.5 mmP x 5.7 mmD x 5 mmH.....	6
70-1069-IMP0018.....	Healing Abutment 4.5 mmP x 5.7 mmD x 7 mmH.....	6
70-1073-PRA0048.....	Temporary Abutment 3.0 mmP.....	6
70-1073-PRA0022.....	Temporary Abutment 3.5 mmP.....	6
70-1073-PRA0024.....	Temporary Abutment 4.5 mmP.....	6
70-1073-PRA0047.....	Temporary Abutment, Non-Engaging, 3.0 mmP.....	6
70-1073-PRA0023.....	Temporary Abutment, Non-Engaging, 3.5 mmP.....	6
70-1073-PRA0025.....	Temporary Abutment, Non-Engaging, 4.5 mmP.....	6

PROSTHETICS - IMPRESSIONS/ANALOGS

70-1072-PRC0055.....	Analog 3.0 mmP.....	7
70-1072-PRC0015.....	Analog 3.5 mmP.....	7
70-1072-PRC0017.....	Analog 4.5 mmP.....	7
70-1072-PRC0051.....	Transfer Coping, Closed-Tray, 3.0 mmP x 3.2 mmD.....	7
70-1072-PRC0053.....	Transfer Coping, Closed-Tray, 3.0 mmP x 3.7 mmD.....	7
70-1072-PRC0007.....	Transfer Coping, Closed-Tray, 3.5 mmP x 3.5 mmD.....	7
70-1072-PRC0009.....	Transfer Coping, Closed-Tray, 3.5 mmP x 4.7 mmD.....	7
70-1072-PRC0011.....	Transfer Coping, Closed-Tray, 4.5 mmP x 4.5 mmD.....	7
70-1072-PRC0013.....	Transfer Coping, Closed-Tray, 4.5 mmP x 5.7 mmD.....	7
70-1072-PRC0052.....	Transfer Coping, Open-Tray, 3.0 mmP x 3.2 mmD.....	7
70-1072-PRC0054.....	Transfer Coping, Open-Tray, 3.0 mmP x 3.7 mmD.....	7
70-1072-PRC0006.....	Transfer Coping, Open-Tray, 3.5 mmP x 3.5 mmD.....	7
70-1072-PRC0008.....	Transfer Coping, Open-Tray, 3.5 mmP x 4.7 mmD.....	7
70-1072-PRC0010.....	Transfer Coping, Open-Tray, 4.5 mmP x 4.5 mmD.....	7
70-1072-PRC0012.....	Transfer Coping, Open-Tray, 4.5 mmP x 5.7 mmD.....	7

PROSTHETICS - TITANIUM SCAN BODIES

70-1073-PRA0080.....	Ti.Scan Body 3.0 mmP.....	7
70-1073-PRA0081.....	Ti.Scan Body 3.5 mmP.....	7
70-1073-PRA0079.....	Ti.Scan Body 4.5 mmP.....	7

PROSTHETICS - LOCATOR ABUTMENT SYSTEM

70-1075-ZST0001.....	35 Ncm Torque Wrench Insert Driver (15 mm).....	13
70-1075-ZST0002.....	35 Ncm Torque Wrench Insert Driver (21 mm).....	13
70-1075-ZST0026.....	Angle Measurement Guide.....	13
70-1075-ZST0004.....	Core Tool (Complete).....	13
70-1075-ZST0003.....	Core Tool Abutment Driver (Gold End).....	13
70-1075-ZST0005.....	Core Tool Abutment Holder Sleeve (4/pk).....	13
70-1075-ZST0006.....	Core Tool Male Removal (Tip End).....	13
70-1075-ZST0025.....	Extended Range Male Processing Package (2/pk).....	13
70-1075-ZST0009.....	Female Analog 4 mmD (4/pk).....	13
70-1075-ZST0007.....	Impression Coping (4/pk).....	13
70-1075-ZST0020.....	Latch Type Torque Wrench Insert Driver (23 mm).....	13
70-1075-ZST0021.....	Latch Type Torque Wrench Insert Driver (29 mm).....	13
70-1075-ZST0065.....	Locator Abutment 3.0 mmP x 1 mmH Cuff.....	12

PARTS INDEX

CODE	DESCRIPTION	PAGE
70-1075-ZST0066	Locator Abutment 3.0 mmP x 3 mmH Cuff	12
70-1075-ZST0011	Locator Abutment 3.5 mmP x 0 mmH Cuff	12
70-1075-ZST0012	Locator Abutment 3.5 mmP x 1 mmH Cuff	12
70-1075-ZST0013	Locator Abutment 3.5 mmP x 2.5 mmH Cuff	12
70-1075-ZST0014	Locator Abutment 3.5 mmP x 3.5 mmH Cuff	12
70-1075-ZST0015	Locator Abutment 4.5 mmP x 0 mmH Cuff	12
70-1075-ZST0016	Locator Abutment 4.5 mmP x 1 mmH Cuff	12
70-1075-ZST0017	Locator Abutment 4.5 mmP x 2 mmH Cuff	12
70-1075-ZST0018	Locator Abutment 4.5 mmP x 3 mmH Cuff	12
70-1075-ZST0019	Locator Abutment 4.5 mmP x 4 mmH Cuff	12
70-1075-ZST0024	Male Processing Package (2/pk)	13
70-1075-ZST0008	Parallel Post (4/pk)	13
70-1075-ZST0010	Processing Spacer (4/pk)	13
70-1075-ZST0022	Square Drive Torque Wrench Insert Driver (15 mm)	13
70-1075-ZST0023	Square Drive Torque Wrench Insert Driver (21 mm)	13

PROSTHETICS - MULTI-UNIT ABUTMENT SYSTEM

70-1074-PRS0001	17° Multi-Unit Abutment 3.5 mmP x 2 mmH	10
70-1074-PRS0002	17° Multi-Unit Abutment 3.5 mmP x 3 mmH	10
70-1074-PRS0003	17° Multi-Unit Abutment 4.5 mmP x 2 mmH	10
70-1074-PRS0004	17° Multi-Unit Abutment 4.5 mmP x 3 mmH	10
70-1074-PRS0005	17° Multi-Unit Abutment 4.5 mmP x 5 mmH	10
70-1074-PRS0006	30° Multi-Unit Abutment 3.5 mmP x 3 mmH	10
70-1074-PRS0007	30° Multi-Unit Abutment 4.5 mmP x 3 mmH	10
70-1074-PRS0008	30° Multi-Unit Abutment 4.5 mmP x 5 mmH	10
70-1074-PRS0031	Angled Multi-Unit Abutment Screw	11
70-1074-PRS0040	Multi-Unit Abutment 3.0 mmP x 1.5 mmH	10
70-1074-PRS0041	Multi-Unit Abutment 3.0 mmP x 2.5 mmH	10
70-1074-PRS0042	Multi-Unit Abutment 3.0 mmP x 3.5 mmH	10
70-1074-PRS0009	Multi-Unit Abutment 3.5 mmP x 1 mmH	10
70-1074-PRS0010	Multi-Unit Abutment 3.5 mmP x 2 mmH	10
70-1074-PRS0065	Multi-Unit Abutment 3.5 mmP x 3 mmH	10
70-1074-PRS0066	Multi-Unit Abutment 3.5 mmP x 5 mmH	10
70-1074-PRS0011	Multi-Unit Abutment 4.5 mmP x 1 mmH	10
70-1074-PRS0012	Multi-Unit Abutment 4.5 mmP x 2 mmH	10
70-1074-PRS0013	Multi-Unit Abutment 4.5 mmP x 3 mmH	10
70-1074-PRS0014	Multi-Unit Abutment 4.5 mmP x 5 mmH	10
70-1074-PRS0016	Multi-Unit Abutment Analog	11
70-1073-PRA0037	Multi-Unit Coping 4.5 mmH, Non-Engaging	11
70-1074-PRS0028	Multi-Unit Driver	11
70-1074-PRS0018	Multi-Unit Gold Bar Coping	11
70-1074-PRS0030	Multi-Unit Gold/Plastic Coping	11
70-1074-PRS0061	Multi-Unit Guide Pin .050" Hex	11
70-1074-PRS0021	Multi-Unit Impression Coping, Closed-Tray	11
70-1074-PRS0052	Multi-Unit Impression Coping, Open-Tray	11
70-1074-PRS0067	Multi-Unit Plastic Coping with Prosthetic Screw .050" Hex	11
70-1072-PRC0014	Multi-Unit Prosthetic Screw .050" Hex	11
70-1074-PRS0015	Multi-Unit Temporary Healing Cap	11
70-1074-PRS0025	Multi-Unit Titanium Temporary	11

PROSTHETICS - SCREWS & GUIDE PINS

70-1072-PRC0002	Guide Pin (5/pk)	9
70-1072-PRC0056	Guide Pin 3.0 mmP (5/pk)	9
70-1072-PRC0001	Titanium Screw	9
70-1072-PRC0003	Titanium Screw (5/pk)	9
70-1072-PRC0058	Titanium Screw 3.0 mmP	9
70-1072-PRC0057	Titanium Screw 3.0 mmP (5/pk)	9

PROSTHETICS - TITANIUM ABUTMENTS

70-1073-PRA0052	Titanium Abutment 3.0 mmP x 4.5 mmH	8
70-1073-PRA0053	Titanium Abutment 3.0 mmP x 6 mmH	8
70-1073-PRA0045	Titanium Abutment 3.5 mmP x 4.5 mmH	8
70-1073-PRA0006	Titanium Abutment 3.5 mmP x 6 mmH	8
70-1073-PRA0046	Titanium Abutment 4.5 mmP x 4.5 mmH	8
70-1073-PRA0008	Titanium Abutment 4.5 mmP x 6 mmH	8

PROSTHETICS - TITANIUM ESTHETIC ABUTMENTS

70-1073-PRA0054	15° Ti. Esthetic Abut., Ant., 3.0 mmP x 1.5 mmH	8
-----------------	---	---

CODE	DESCRIPTION	PAGE
70-1073-PRA0059	15° Ti. Esthetic Abut., Ant., 3.0 mmP x 2.3 mmH	8
70-1073-PRA0009	15° Ti. Esthetic Abut., Anterior, 3.5 mmP	8
70-1073-PRA0031	15° Ti. Esthetic Abut., Anterior, 3.5 mmP x 1.5 mmH	8
70-1073-PRA0010	15° Ti. Esthetic Abut., Anterior, 4.5 mmP	8
70-1073-PRA0062	15° Ti. Esthetic Abut., Anterior, 4.5 mmP x 1.5 mmH	8
70-1073-PRA0013	15° Ti. Esthetic Abut., Posterior, 4.5 mmP	8
70-1073-PRA0055	Ti. Esthetic Abut., Anterior, 3.0 mmP x 1.5 mmH	8
70-1073-PRA0060	Ti. Esthetic Abut., Anterior, 3.0 mmP x 2.3 mmH	8
70-1073-PRA0011	Ti. Esthetic Abut., Anterior, 3.5 mmP	8
70-1073-PRA0032	Ti. Esthetic Abut., Anterior, 3.5 mmP x 1.5 mmH	8
70-1073-PRA0012	Ti. Esthetic Abut., Anterior, 4.5 mmP	8
70-1073-PRA0063	Ti. Esthetic Abut., Anterior, 4.5 mmP x 1.5 mmH	8
70-1073-PRA0014	Ti. Esthetic Abut., Posterior, 4.5 mmP	8
70-1073-PRA0015	Ti. Esthetic Abut., Posterior, Wide, 4.5 mmP	8

PROSTHETICS - UCLA ABUTMENTS

70-1073-PRA0056	UCLA Gold Abutment, 3.0 mmP	9
70-1073-PRA0027	UCLA Gold Abutment, 3.5 mmP	9
70-1073-PRA0029	UCLA Gold Abutment, 4.5 mmP	9
70-1073-PRA0058	UCLA Plastic Abutment, 3.0 mmP	9
70-1073-PRA0018	UCLA Plastic Abutment, 3.5 mmP	9
70-1073-PRA0020	UCLA Plastic Abutment, 4.5 mmP	9
70-1073-PRA0057	UCLA Plastic Abutment, Non-Engaging, 3.0 mmP	9
70-1073-PRA0019	UCLA Plastic Abutment, Non-Engaging, 3.5 mmP	9
70-1073-PRA0021	UCLA Plastic Abutment, Non-Engaging, 4.5 mmP	9

INCLUSIVE MINI IMPLANT SYSTEM

IMPLANTS

70-1068-IMP0001	Mini Implant O-Ball 2.2 mmD x 10 mmL	19
70-1068-IMP0002	Mini Implant O-Ball 2.2 mmD x 13 mmL	19
70-1068-IMP0003	Mini Implant O-Ball 2.2 mmD x 15 mmL	19
70-1068-IMP0004	Mini Implant O-Ball 2.5 mmD x 10 mmL	19
70-1068-IMP0005	Mini Implant O-Ball 2.5 mmD x 13 mmL	19
70-1068-IMP0006	Mini Implant O-Ball 2.5 mmD x 15 mmL	19
70-1068-IMP0007	Mini Implant O-Ball 3.0 mmD x 10 mmL	19
70-1068-IMP0008	Mini Implant O-Ball 3.0 mmD x 13 mmL	19
70-1068-IMP0009	Mini Implant O-Ball 3.0 mmD x 15 mmL	19

PROSTHETICS

70-1066-MNI0001	Blockout Shims (25/pk)	20
70-1066-MNP0004	Impression Coping (4/pk)	20
70-1066-MNP0007	Instrumentation O-Rings 2.5 mm x 1 mm (5/pk)	20
70-1066-MNP0005	Mini Implant Replica (4/pk)	20
70-1066-MNP0006	O-Ring Housing	20
70-1066-MNP0008	Prosthetic O-Rings 3/16" x 1/16" (10/pk)	20

INSTRUMENTATION

70-1071-SRG0008	Cortical Bone Drill Ø1.5 mm	23
70-1071-SRG0010	Cortical Bone Drill Ø1.7 mm	23
70-1071-SRG0012	Cortical Bone Drill Ø2.4 mm	23
70-1067-MNI0001	Handpiece Mini Implant Driver 13 mm	23
70-1067-MNI0002	Handpiece Mini Implant Driver 5 mm	23
70-1067-MNI0004	Mini Implant Driver 13 mm	23
70-1067-MNI0003	Mini Implant Driver 5 mm	23
70-1067-MNI0007	Radiographic Template	23
70-1067-MNI0006	Surgical Instrumentation Kit	22

INCLUSIVE[®]

DENTAL IMPLANT SYSTEM



Designed & Manufactured
in the USA



PRISMATIK
DENTALCRAFT, INC.

2144 Michelson Drive • Irvine, CA 92612, USA